

CALIBRATION OF RADIOCARBON AGE TO CALENDAR YEARS

(Variables: C13/C12=-7.5;lab. mult=1)

Laboratory number: **Beta-193850**


Conventional radiocarbon age: **900±40 BP**

2 Sigma calibrated result: Cal AD 1030 to 1230 (Cal BP 920 to 720)
(95% probability)

Intercept data

Intercept of radiocarbon age
with calibration curve: **Cal AD 1160 (Cal BP 790)**

1 Sigma calibrated result: Cal AD 1040 to 1190 (Cal BP 910 to 760)
(68% probability)

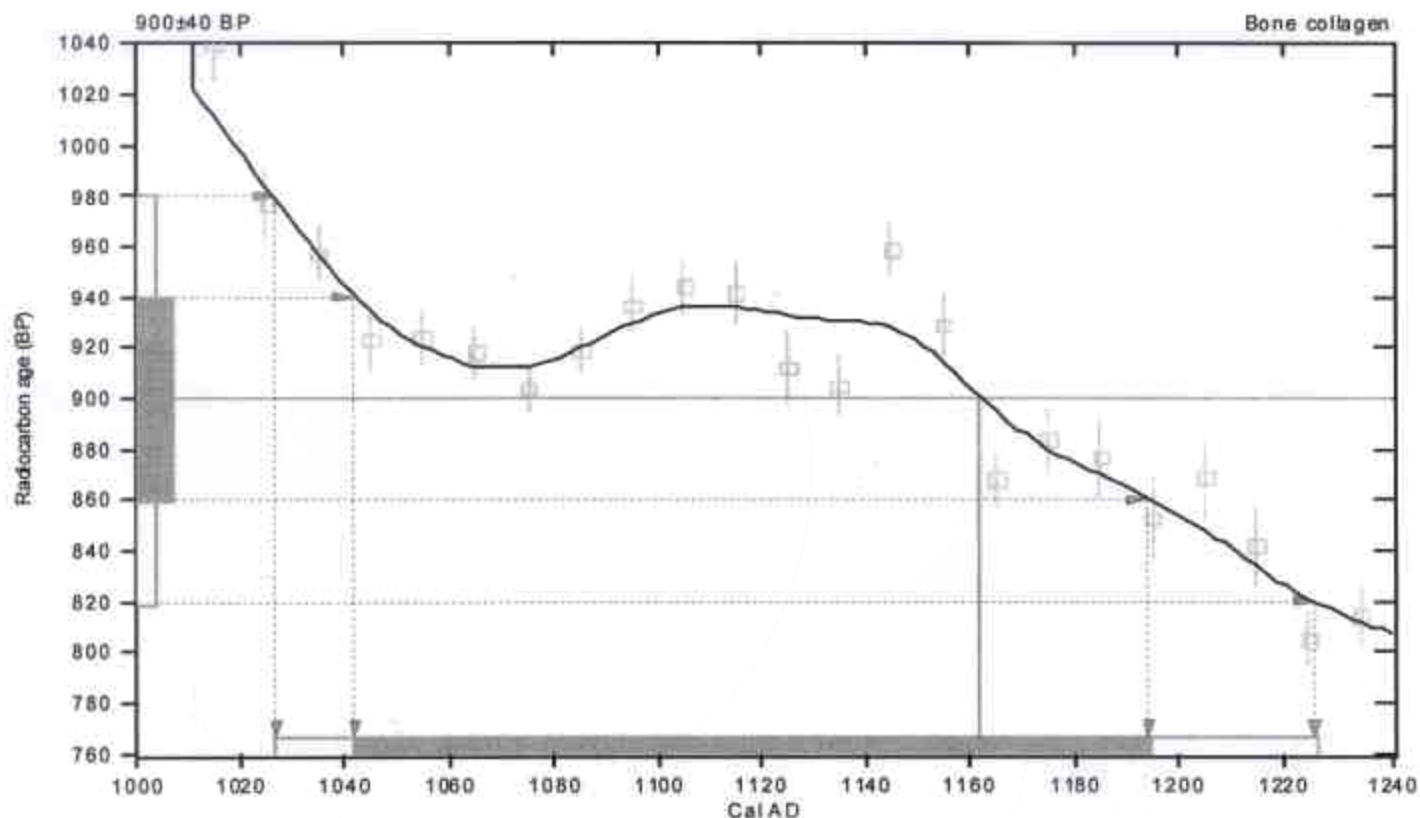

References:

Database used

INTCAL98

Calibration Database

Editorial Comment

Stuiver, M., van der Plicht, H., 1998, *Radiocarbon* 40(3), pxi-xii

INTCAL98 Radiocarbon Age Calibration

Stuiver, M., et al., 1998, *Radiocarbon* 40(3), p1041-1083

Mathematics

A Simplified Approach to Calibrating C14 Dates

Talma, A. S., Vogel, J. C., 1993, *Radiocarbon* 35(2), p317-322

Beta Analytic Radiocarbon Dating Laboratory

4985 S.W. 74th Court, Miami, Florida 33155 • Tel: (305)667-5167 • Fax: (305)663-0964 • E-Mail: beta@radiocarbon.com